8 rue des Frères Montgolfier
49240 Avrillé
France

Tel : +33(0) 2 41 17 49 49
Fax : +33(0) 2 72 22 11 43

Instructions for Use

Rev : V3
September 2025

ACC1349TUC & ACC1349TUC2 "factory roof" type accessories

Use, cleaning and maintenance of our "factory roof" type accessories

Our factory roof accessories are available in two versions: 3 steps (ACC1349TUC) and 4 steps (ACC1349TUC2), to best arrange your patient's ankle for knee surgery.

Restrictions on Use

- The user must ensure that the type of "factory roof" and its material is suitable for the desired position for the patient.
- These accessories are intended for users trained in patient positioning and the risk of pressure ulcers.
- Do not wash mattresses or fixing rods in the washing and disinfection booth.
- Never use abrasive cleaners or scraper sponges.
- Do not attach sticky strips to mattresses or the upper.
- If an alcohol-based product for disinfecting the patient's skin is used, it is imperative for safety reasons (risk of inflammation and/or maceration), to ensure that it does not accumulate under the patient.
- The rod is designed for fixing operating tables to current standards.

Washing, disinfection and maintenance

- Factory roof cushions with their stems can be cleaned by wiping with a soft cloth dampened with water containing a neutral detergent or with a ready-to-use solution (e.g. ANIOS Surfa'safe, ALFAKARM Septalkan, HUCKERT'S Umonium 38 Medical Spray...) or soaked wipes (e.g. ANIOS Oxy Wipes; Wip'ANIOS Excel; HUCKERT'S Umonium 38 Medical Tissues Laboratory...).
- In general, surface disinfectants containing a set of active ingredients such as aldehyde, quaternary compounds, guanidine derivatives and active oxygen, have proven their effectiveness. But always choose those formulated specifically for equipment, less film-forming and aggressive.
- In situ cleaning and disinfection can also be carried out on the coating with hot water by hand and a neutral detergent or with a sodium hypochlorite solution (0.1% or 1000 parts per million of available chlorine).
- Products such as Ercesolvent©, Remove©, GILBERT Non-Stick,© etc. used to remove adhesive residues (Elastoplast©, sticky drapes), should be thoroughly rinsed and dried immediately after use. Failure to do so may result in the buildup of reagent damaging mattress components. All products based on acetone, ether and other volatile solvents must be used with the same precautions.
- It is essential that mattresses and uppers dry thoroughly after cleaning.
- It is strongly recommended to clean the different surfaces of mattresses and rods between two patients, and systematically after a septic procedure.
- Finally, it is imperative for hygiene reasons to replace the cushion as soon as it shows damage (tear, cut, cracks, burns, etc.) Indeed, the altered products are no longer waterproof and the moisture that then penetrates the foam promotes the development of germs and bacteria.

Special precautions

Before any use, it is necessary to ensure that the cushion and its stem as well as the clam (not supplied) are in good condition, that they are positioned flat and that they are properly placed on the mattress and the table rail.

The factory roof mattress and the operating table cushion must be perfectly dry.

The use of this mattress is not a substitute for the monitoring necessary to keep the patient on the support and to prevent bedsores.

8 rue des Frères Montgolfier
49240 Avrillé
France

Tel : +33(0) 2 41 17 49 49
Fax : +33(0) 2 72 22 11 43

Instructions for Use

Rev : V3

September 2025

Pressure ulcer prevention requires identifying risk factors and planning changes in position every 2 to 3 hours, or even at a higher frequency and at least specific visual monitoring.

Installation of the "factory roof" cushion with its stem.

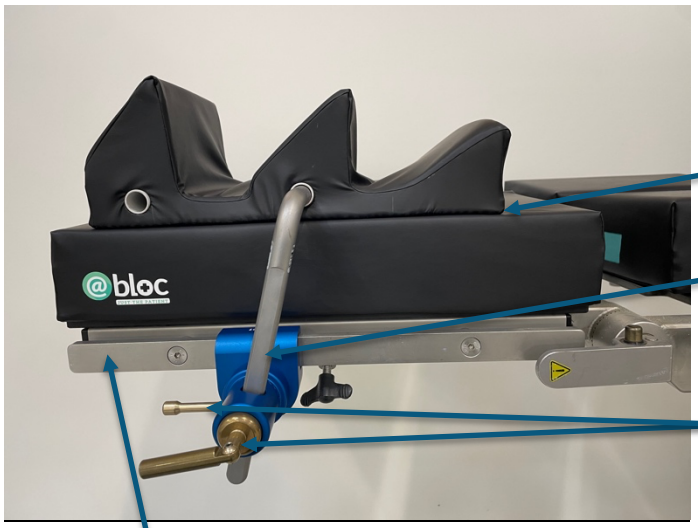

Make sure that the cushion rests on the mattress to avoid any risk of the cushion falling.

Make sure that the flat of the rod is positioned in front of the axis of the clamp that will perform the tightening.

Make sure that the clasp is sufficiently tight on the stem to prevent any possible slippage during surgery. The same goes for the clamping of the clamp on the rail.

The clamp must not be clamped on the end of the free limit of the rail under any circumstances.

Special conditions of storage and use

Min temperature	Storage : -15 °	Use : + 15°
Max temperature	Storage : + 45 °	Use : +25°
Hygrometry (%HR) min	Storage : 30%	Use : 30%
Hygrometry (%HR) max	Storage : 70%	Use : 70%

Spare parts

Only the reference rod is available as a spare part: GeFixUsl.

End of life

At the end of life:

- The cushion must be cleaned and disinfected normally and then placed in the system intended for the disposal of run-of-mine waste
- The rod is to be placed in the metal recycling system.

Normative references

Manufacturer: @bloc

Complies with European regulations

CE Class 1 Medical Device

8 rue des Frères Montgolfier
49240 Avrillé
France

Tel : +33(0) 2 41 17 49 49
Fax : +33(0) 2 72 22 11 43

Instructions for Use

Rev : V3

September 2025

Depending on the fabric used: Flammability BS7175 1989 - Antistatic BS2050 1978 - ISO 2878.

Any serious incident that occurs in connection with one of our cushions must be notified to @bloc and the ANSM in accordance with the regulations in force.

For any further information, please contact us.

CE

Authorised Representative for Switzerland:

CH REP

GMB Services SA
Route de Mouthe 20,
1343 Les Charbonnières - Switzerland
info@gmb-services.com

Swiss Importer:

GMB Services SA
Route de Mouthe 20,
1343 Les Charbonnières - Switzerland